

Lovibond® Water Testing

Tintometer® Group



The Measurement Comparability Between the PTV 1000 White Light LED Turbidimeter and the 1720E at a Colorado, Partnership Water Plant

By Michael J. Sadar
December 12, 2016

Introduction:

The goal of this study was to collect comparability data between the Lovibond® PTV 1000 White Light LED turbidimeter and the HACH® 1720E turbidimeter. The instruments were to be set up and run as filter effluent turbidimeters and to capture continuous turbidity measurements through several consecutive filter runs. The second goal was to spike the filter effluent with settled water to study the response level and response time for these two test instruments.

Background:

This comparability study focused on water produced at a Partnership for Safe Drinking Water Filtration Plant is located near the metropolitan of Denver, Colorado. The raw water was surface water from the South Plant River Basin that was characterized with high levels of total dissolved solids and micro pollutants such as pharmaceutical residuals. The water was treated through a multibarrier process that included riverbank filtration, aquifer recharge and recovery, precipitative softening, ultraviolet light coupled with advanced peroxidase oxidation, biological activated carbon filtration and activated carbon adsorption. The filtration stage is through a dual media anthracite filter. The water plant was commissioned in 2010 and has a treatment capacity of 50 million gallons per day.

Prior to this study, the plant had been off line to allow for the addition of additional filters. The water plant recently came back on line but was not in what was a considered a state of optimization. The plant has turbidity limit of 0.08 NTU on the filters, and normal operation of the filters is to produce water that is below 0.030 NTU. The filter effluent (FE) from one of the new filters was the monitoring point for this comparability study.

Materials and Methods:

Two instruments were installed side-by-side on the FE sample tap. One instrument was the PTV 1000 White Light Turbidimeter. The second instrument was the HACH® 1720E turbidimeter. Both instruments had less than one month of use. Installation was according to each manufacturer's respective recommendations and included the following important protocols:

- Instruments were run for approximately 7 days prior to the study to allow for proper wetting of surfaces. This ensured that internal bubble reflections were minimized.
- Sample lines were the same distance from the tap and ran parallel to each instrument.
- Sample flow rates were 60-ml/minute on the PTV 1000 and 250 ml/minute on the 1720E.
- Signal averaging was set to the same value on both instruments.
- Bubble removal algorithms were turned on with respect to both instruments.
- The 1720E was allowed to run for 24-hours to ensure lamp stability prior to calibration.
- Both instruments underwent the zero-electronics operation prior to calibration.
- Both instruments were calibrated according to the respective calibration procedures. The 1720E used a fresh prepared 20.0 NTU formazin standard. The PTV 1000 used a fresh prepared 5.0 NTU calibration standard.
- After calibration and prior to data collection both instruments were verified on fresh prepared formazin standards. Two verification standards were prepared, one at 1.0 NTU and the second at 0.6 NTU. Both instruments passed the pass/fail criteria of $\pm 10\%$ of the value of the standard or 0.03 NTU, whichever was greater. The verification was repeated at the completion of the study, and again both instruments passed the verification protocol.
- Both Instruments were set to the same data log interval, which was once every 15-seconds
- Measurements were logged via Modbus protocol (digitally) to a dedicated computer.

Data and Results:

The measurements from each instrument were recorded for approximately 67 hours of continuous monitoring of the CFE stream. This period encompassed approximately four complete filtration cycles (ripening through backwash). Figure 1 is the graphical presentation of the data from the PTV 1000 and 1720E instruments. The PTV 1000 trace is dark blue and the 1720E trace is brown. The vertical red lines represent the time the data was valid. Immediately prior and after these lines was when the quality assurance verifications were performed. The graph is scaled from 0 to 0.30 NTU, with the maximum representing the USEPA regulatory limit of turbidity for filter effluent water.

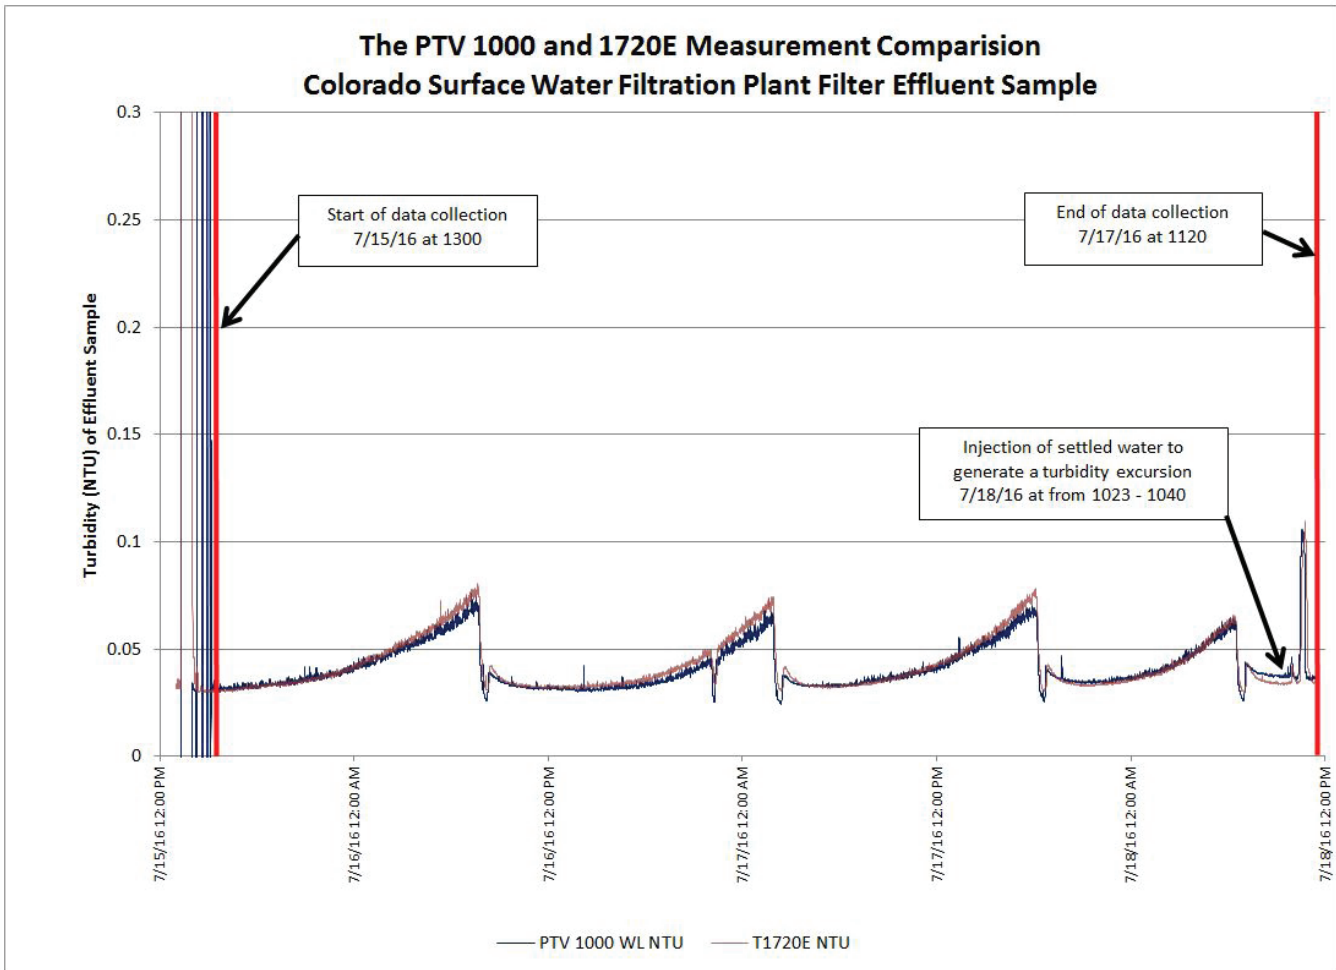


Figure 1 - Graphical Presentation of the On-line monitoring of filter effluent sample using the PTV 1000 and 1720E Turbidimeters

Figure 1 illustrates that both instruments track each other over the course of this study. This included the changes in turbidity that were expected through ripening, on-line production and termination of the run. The turbidities ranged from a low of approximately 0.030 NTU to a high of approximately 0.1 NTU. The graph contains 16087 data points for each instrument. From a statistical perspective, the averaged PTV 1000 reading was 0.042 NTU and the 1720E was 0.043 NTU. The net difference is well within the stated specifications of each instrument which is ± 0.015 NTU (the stated accuracy below 1 NTU). The instruments demonstrated similar precision, with standard deviations that were very similar. Table 1 below provides a summary of the study.

	1720E (NTU)	PTV 1000 (White LED) (NTU)
Average	0.043	0.042
Standard Deviation	0.0122	0.0107
N	16087	16087

This study also included a simplistic spike of some raw water into the effluent stream. The intent of the spike was to generate a more severe change in turbidity that would be subject to detection between the two turbidimeters. Figure 2 is a graphical illustration of the spike itself. The blue trace is the PTV 1000, and the brown trace is the 1720E. The y-axis is scaled from 0 to 0.30 NTU.

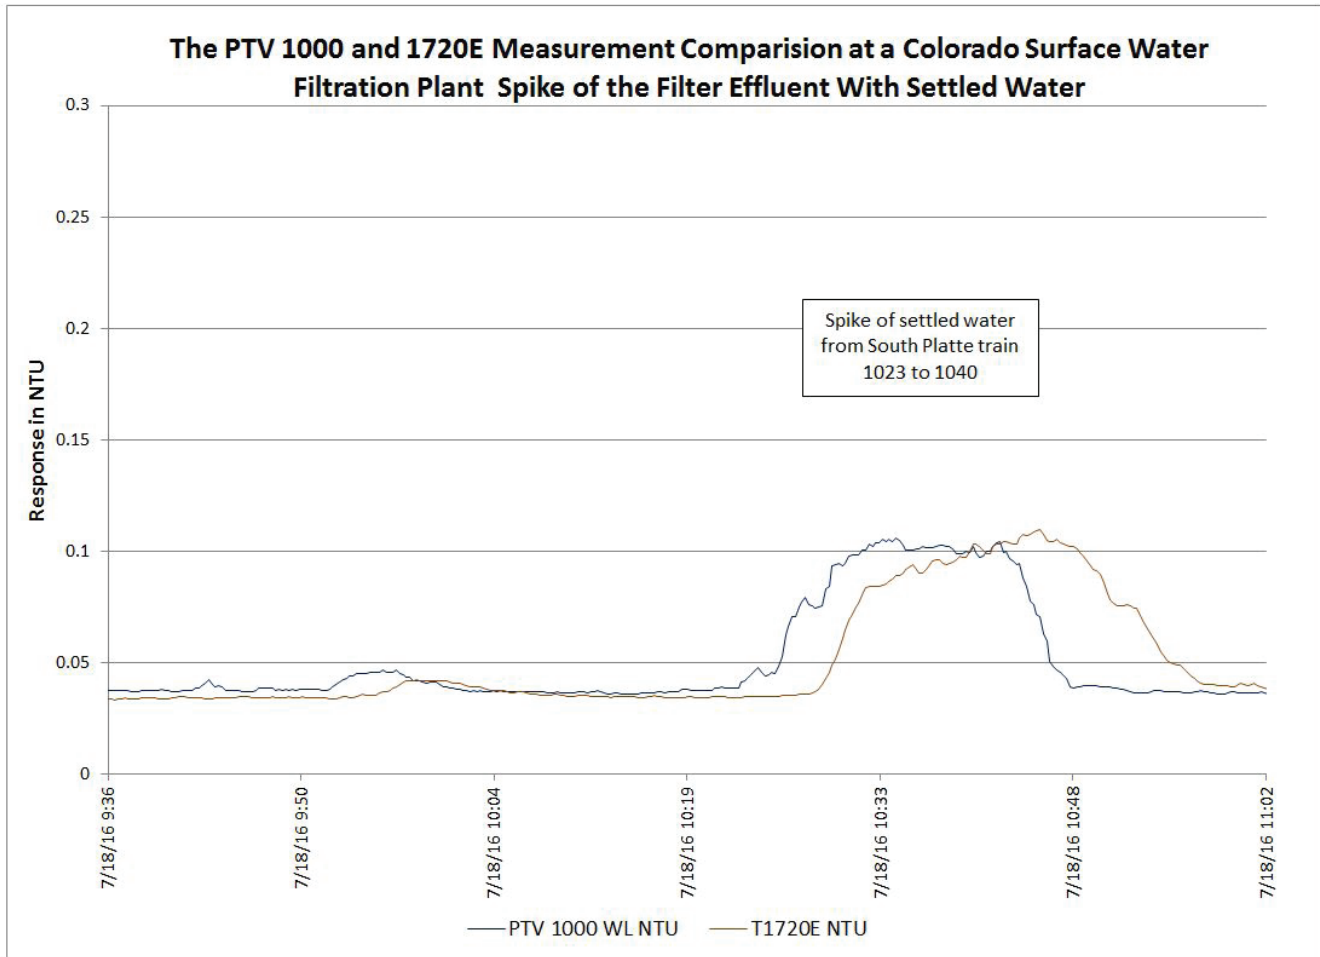


Figure 2 – Graphical plot of the PTV 1000 and 1720E responsiveness to a spike of settled water into the filter effluent stream.

In this graph, both instruments demonstrate the same magnitude of response to the spike of settled water. The graph does show that the PTV 1000 does have a faster response and recovery to the spike when compared to the 1720E turbidimeter. This is a factor of the flow rates to the each instrument, but it is important to note that even though the 1720E has more than 4 times the flow rate of the PTV 1000, its response time is still slower (250 ml/minute flow for the 1720E and 60 ml/minute for the PTV 1000). This can play an important role as water plants use every means necessary to conserve water both internal and external of the filtration plant.

Conclusions:

The comparability study between the PTV 1000 White Light LED turbidimeter and the Hach 1720E turbidimeter was successfully carried out at a highly recognized drinking water filtration plant. The instruments continuously monitored and logged turbidity data for several continuous filter runs, collecting more than 16,000 consecutive data points for each instrument. Over the duration of the study, the instrument measurements averaged within 0.001 NTU of each other, which was within the accuracy specifications for each instrument. The study demonstrated that a significant spike of turbidity was also comparable with respect to the magnitude of response on both instruments. The spike did demonstrate that the PTV 1000 required a sample flow rate that was for times lower than the 1720E to yield an equivalent response time. This will have a substantial impact on sample consumption over time.

HACH is a registered trademark of HACH Company, Loveland, CO.

Tintometer GmbH.
Tel: +49 (0) 231/94510-0
sales@tintometer.de
Germany

Tintometer Brazil
sales@tintometer.us
Brazil

Tintometer Inc.
Tel: +1 941 756 6410
sales@tintometer.us
U.S.A.

Tintometer AG
info@tintometer.ch
Switzerland

The Tintometer Ltd.
Tel: +44 1980 664800
water.sales@tintometer.com
UK

Tintometer South East Asia
lovibond.asia@tintometer.com
Malaysia

Tintometer India Pvt. Ltd.
Tel: 1800 102 3891
indiaoffice@tintometer.com
India

Tintometer China
Tel: +86 10 85251111 ext.330
China